

RAININ

Pipetting 360°

Pipet-Lite®

Adjustable Spacer

**Multichannel Pipette
with Adjustable Nozzle Spacing
and LTS® LiteTouch™ Tip Ejection**

**6 or 8
channels**

**Models:
LA8-50
LA6-300
LA8-300
LA6-1200
LA8-1200**



METTLER TOLEDO

Introduction

This is an addendum to the Pipet-Lite manual (9920-237) which describes general pipette operation, modes, and options. Pipet-Lite Adjustable-Spacer multichannel pipettes are based on Pipet-Lite single-channel models, and operate in the same way. Two versions of the adjustable-nozzle multichannel Pipet-Lite pipette are available: **6-channel (LA6)** and **8-channel (LA8)**, with nozzle spacing adjustment ranges shown below:

6-channel	9 mm to approx. 19 mm
8-channel	9 mm to approx. 14 mm

6- and 8-channel versions are available in the volume ranges: 20-300 μL and 100-1200 μL . 8-channel versions are also available in the 5-50 μL volume range.

Packing List

In addition to this manual, the pipette box should contain:

Pipet-Lite instruction manual 9920-237, Rainin Test Report, Performance Assurance Brochure, sample tips.

Spacing Controls and Indicators

Nozzle spacing is changed with the use of two knurled knobs on either end of the liquid end manifold: the LIMITER knob and the SPACING ADJUSTMENT knob.

The LIMITER knob (marked with the nozzle spacing range) sets the desired maximum spacing within the pipette's spacing range. A vertical arrow at the top of the knob on the liquid end manifold is the set point.

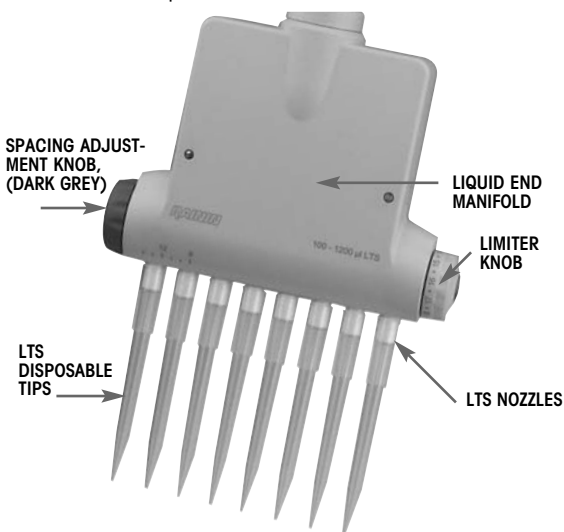


FIGURE 1 NOZZLE SPACING CONTROLS

When you have set the maximum spacing with the LIMITER knob, turn the SPACING adjustment knob to open the nozzle spacing to the set value. A scale on the liquid end manifold gives a visual reference of the set spacing. Simply line up the the leftmost nozzle with the scale on the manifold, as shown here.



The full range of adjustment for the eight-channel version is shown below. Nozzles are set to 9 mm spacing on the left and 14 mm spacing on the right.



Minimum spacing



Maximum spacing

FIGURE 2: NOZZLE SPACING RANGE

Positioning the Liquid End Manifold

The liquid end manifold can be rotated to any angle for convenience. You do not need to loosen the coupling nut.

When in use, it is recommended to hold the Pipet-Lite handle in your dominant hand and turn the adjustment knob with your other hand. Right-handed users should position the pipette as shown on the cover.

If you are left-handed, you can rotate the liquid end manifold 180° clockwise, so that the adjustment knob can be manipulated with your non-dominant hand.

Tip Selection

Pipet-Lite multichannel pipettes must use RAININ LTS tips.

LA8-50: use 250 μ L LTS tips

LA6-300 and LA8-300: use 300 μ L LTS tips

LA6-1200 and LA8-1200: use 1200 μ L LTS tips (recommended) or 1000 μ L LTS tips – picks up 1200 μ L (except aerosol-resistant)

LTS tips have a cylindrical cross-section with a well-defined seal ring, thin wall, and positive stop. They seal properly on the LTS nozzles and cannot be jammed or forced too far onto the nozzles.

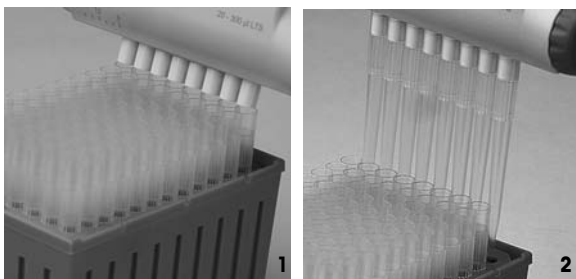


FIGURE 3: MOUNTING TIPS

Mounting LTS Tips

Mounting racked LTS tips onto LA6 and LA8 pipettes is simple.

1. Set the nozzle spacing to 9 mm (same as the spacing for racked tips) by rotating the dark grey SPACING ADJUSTMENT knob fully clockwise.
2. Align the nozzles into the row of tips, holding the pipette at a slight angle. (Figure 3.1). Rotate the pipette upright and press the nozzles into the tips until the “positive stop” is reached. The tips are now mounted with proper sealing. You do not need to hand-tighten, use heavy pressure, or “rock” the nozzles onto the tips to obtain a good seal. Withdraw the tips from the tip rack. (Figure 3.2)

Setting the Nozzle Spacing

With tips mounted on the nozzles, and before you begin to aspirate sample:

- If you know the spacing for the receiving wells or test-tube block, set this value on the LIMITER knob.
- If you do not know the spacing, hold the pipette so that the tip ends are above the centers of the wells or test-tube block into which you will dispense. Look at the scale on the liquid end manifold, and note where the marked nozzle aligns. Set this value on the LIMITER knob.
- If you accidentally over-extend the spacing, you can click the LIMITER knob to smaller values, stopping when the tip ends are aligned over the centers of the wells/test tubes.

Once the LIMITER knob has been set, spacing the nozzles properly is simple.

Just pick up sample, set the nozzle spacing by moving the SPACING ADJUSTMENT knob until it stops at the value set by the LIMITER knob, and dispense into the wells or test-tube block.

Tip Immersion Depth

The recommended depth for tip insertion into the sample for each Pipet-Lite adjustable-nozzle multichannel model is shown in the table below.

<u>Model</u>	<u>Immersion Depth</u>
LA8-50	2 - 3 mm
LA6-300, LA8-300	3 - 6 mm
LA6-1200, LA8-1200	6 - 10 mm

Tip immersion depth is important. If exceeded, the measured volume may be inaccurate, possibly out of specification.

Tip angle: Operate the pipette within 20 degrees of vertical.

Tip Ejection

Simply press on the tip ejector button. All tips are ejected cleanly with minimal pressure on the thumb.

Specifications

These manufacturer's specifications should be used as guidelines when establishing your own performance specification.

Model	Volume μL	Increment μL	Accuracy		Precision	
			%	μL (±)	%	μL (≤)
LA8-50 (range 5-50 μL)	5	0.05	3.5	0.18	1.5	0.075
	25		1.2	0.30	0.4	0.1
	50		0.8	0.40	0.2	0.1
LA6-300, LA8-300 (range 20-300 μL)	30	0.5	2.5	0.75	1.0	0.3
	150		0.8	1.2	0.25	0.375
	300		0.8	2.4	0.15	0.45
LA6-1200, LA8-1200 (range 100-1200 μL)	100	2.0	3.6	3.6	0.60	0.60
	600		0.8	4.8	0.20	1.20
	1200		0.8	9.6	0.15	1.80

(Specifications subject to change without notice)

Care and Maintenance

Pipet-Lite Adjustable Spacer Multichannel pipettes are precision devices and should be treated with the degree of care appropriate for laboratory instrumentation.

When not in use it is recommended to store the pipette safely in one of the accessory stands listed in Ordering Information. Do not drop the pipette, or store the pipette flat if tips with liquid are mounted.

No user maintenance is required except for occasional cleaning: wipe the pipette with a clean cloth dampened with distilled water.

Service

If you experience any problems with your Pipet-Lite multichannel pipette contact RAININ Technical Support at 800-543-4030. If you are located outside North America please refer to the numbers listed on the back page.

Ordering Information

Cat. No. **Description**

Pipettes:

LA8-50	8-channel, 5 μ L to 50 μ L
LA6-300	6-channel, 20 μ L to 300 μ L
LA8-300	8-channel, 20 μ L to 300 μ L
LA6-1200	6-channel, 100 μ L to 1200 μ L
LA8-1200	8-channel, 100 μ L to 1200 μ L

Note: LTS multichannel pipettes require LTS tips.

Accessories:

HU-M3	Package of 3 Magnetic Hang-Ups. Includes adhesive disk for attachment to a non-ferrous vertical surface
HU-S3	Shelf clamp with 3 Hang-Ups attached
CR-7	Free-standing Pipette Carousel, for up to 7 pipettes
HU-A3	Multichannel Adapter for HU-M3, HU-S3 & CR-7. Set of 3

**To order pipettes or accessories, call 800-472-4646,
or visit www.rainin.com on the web.**

RAININ, Pipet-Lite, and LTS are registered trademarks, and LiteTouch and Hang-Ups are trademarks of Rainin Instrument, LLC. Pipet-Lite: U.S. Patent Nos. 5,614,153; 5,700,959; 5,849,248. Tip/Shaft System: For use under U.S. Patent Nos. 6,168,761 B1; 6,171,553 B1; 6,568,288 B2; 6,737,023 B1; 6,745,636 B2; 6,967,004 B2. Other U.S. and national patents pending. Prices and specifications subject to change without notice.

Limited Warranty

See the Limited Warranty and Limitations of Liability Statement. Please complete and return the Warranty Registration Card on receipt of your pipette.

RAININ pipettes are calibrated with RAININ tips. To assure excellent reproducibility and performance, use only RAININ tips as recommended in this manual. Specified performance is guaranteed only when RAININ tips are used.

Contacting RAININ

Technical Information:

T: 800-543-4030 F: 510-564-1617 tech.support@rainin.com

Pipette Service:

T: 800-662-7027 F: 781-935-7631 service@rainin.com

Direct Order Line:

T: 800-472-4646 F: 510-564-1617 pipets@rainin.com

RAININ website: www.rainin.com

From outside North America: T: +1-510-564-1600

www.mt.com/rainin

global@rainin.com (from outside the U.S.)

METTLER TOLEDO Offices

METTLER TOLEDO website: www.mt.com/rainin

Mettler-Toledo (Schweiz) GmbH, Im Langacher , 8606 Greifensee CH

Verkauf 044 944 45 45 salesRN.ch@mt.com

Service 044 944 47 47 serviceRN.ch@mt.com

Mettler Toledo GmbH, Ockerweg 3 , 35396 Giessen DE

Verkauf +49 641 507 222 info.mtd@mt.com

Service +49 641 507 307 info.mtd@mt.com

Mettler-Toledo SAS, 18-20 avenue de la Pépinière , 78220 Viroflay FR

Ventes 01 30 97 17 17 marcom.fr@mt.com

Laboratoire d'Etalonnage Accrédité,

264 rue Abraham Lincoln Service Pipette, 62400 Bethune FR

Service 03 21 64 54 66 marcom.fr@mt.com

N.V. Mettler-Toledo S.A., Leuvensesteenweg 384 , 1932 Zaventem BE

Sales +32 2334 0211 general.mtb@mt.com

Service +32 2334 0211 general.mtb@mt.com

Mettler-Toledo S.A.E., Miguel Hernández 69-71 ,

08908 L'Hospitalet de Llobregat (Barcelona) ES

Ventas 0034 93 223 7666 mtemkt@mt.com

Servicio Técnico 0034 93 223 7666 mtemkt@mt.com

Mettler-Toledo A/S, Naverland 8 , 2600 Glostrup DK

Salg 43 27 08 25 info.mtdk@mt.com

Service 43 27 08 25 info.mtdk@mt.com

Rainin Instrument, LLC

7500 Edgewater Drive, Box 2160, Oakland, CA 94621-0060

a METTLER TOLEDO Company

Prices and specifications are subject to change without notice.

Copyright 2008, Rainin Instrument, LLC.

9920-356 REV B